


SET-UP AND CALIBRATION INSTRUCTIONS FOR ADJUSTABLE MODELS

All IRt/c models with the “A” designator (example: IRt/c.10A-K-LoE) can be field calibrated for the specific requirements of the application to precisely indicate the actual temperature of the target, and to correct for reflective errors caused by ambient variations (see Tech Note #64).

The basic operation of the IRt/c adjustment is to rescale the signal output until it matches the actual temperature for the thermocouple type in use. In the vicinity of the calibration point, the output will match the linearity of the t/c. When the adjustment is made to actual temperature, the Automatic Ambient Compensation System is automatically correctly scaled.

The above chart shows the actual performance of a .10A-HiE model as an illustration of the effect of adjustment on the signal.

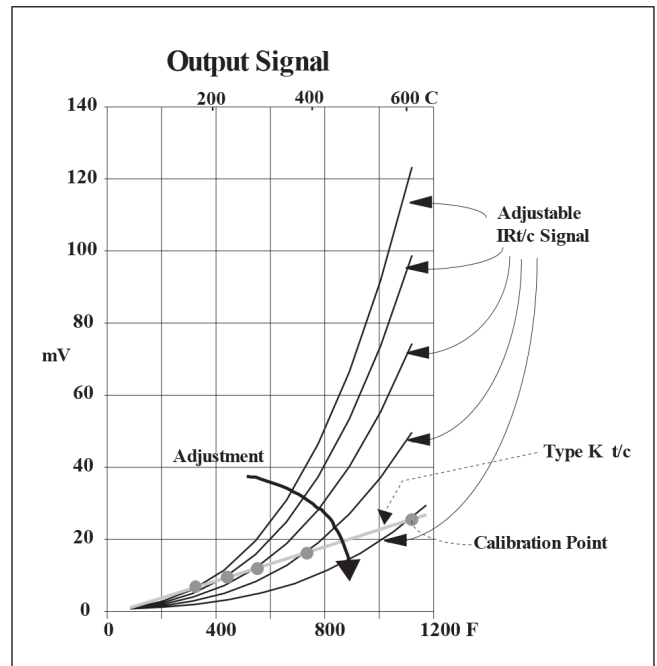

Exergen Global offices:

The Netherlands
Pastoor Clercxstraat 26
5465 RH Veghel
Tel: +31(0) 413 37 65 99
Fax: +31(0) 413 37 93 10

USA
400 Pleasant Street
Watertown, MA 02472
Tel: +1 617 649 6322
Fax: +1 617 923 9911

office@exergenglobal.com
www.exergenglobal.com